



Test Report

Number: GZHT02286854

Report Ref:	GZHT02286854		
Date Received:	Apr 30, 2020	Date Issued:	May 14, 2020

--	--	--	--

The Following Sample Was Submitted And Identified By/On Behalf Of The Applicant As:			
End Uses	:	Non-Sterile Medical Face Mask	
Ratings	:	Type IIR	
Sample Name	:	Medical Mask	
Size	:	17.5*9.5cm	
Colour	:	Blue	
Standard	:	EN 14683:2019+AC:2019	
Manufacturer	:	REDACTED	
Ref	:	REDACTED	
Date received/ Test Started	:	Apr 30, 2020	

Prepared And Checked By:
For Intertek Testing Services Shenzhen Ltd. Guangzhou Branch

Lin Lin
General Manager



Ula / hilaryxu


Intertek Testing Services Shenzhen Ltd. Guangzhou Branch

深圳天祥质量技术服务有限公司广州分公司


Room 02, 1-8/F & Room 01, E101/E201/E301/E401/E501/E601/E701/E801, Hengyun Building, 235 Kaifa Ave., Guangzhou
 No.7-2, Caipin Road, Guangzhou Science City, GETDD, Guangzhou, China Economic & Technological Development District, Guangzhou, China
 中国广州经济技术开发区科学城彩频路7号之二第1-8层02房、01房 中国广州经济技术开发区开发大道235号恒运大厦3楼
 101、
 E201、E301、E401、E501、E601、E701、E801 Tel: +86 20 8396 6868 Fax: +86 20 8222 8169 Postcode: 510730
 Tel: +86 20 8213 9001 Fax: +86 20 8208 9909 Postcode: 510663



Original Sample Photo

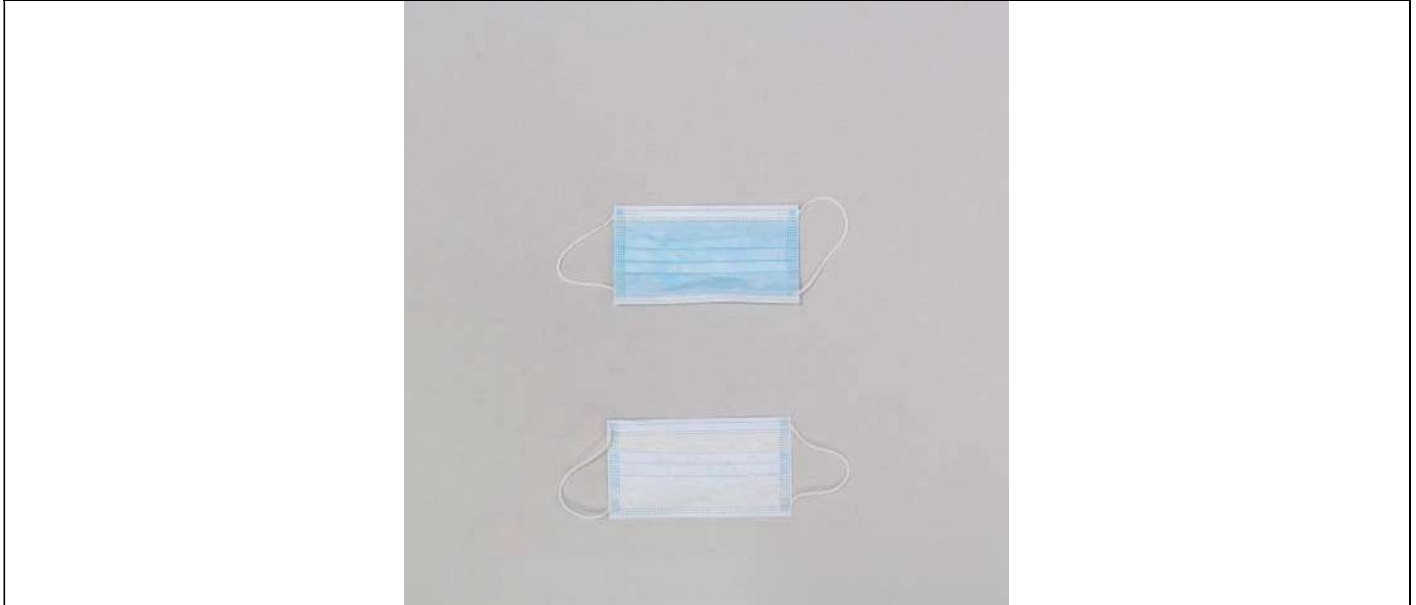

Prepared And Checked By:
For Intertek Testing Services Shenzhen Ltd. Guangzhou Branch



Lin Lin
General Manager



Ula / hilaryxu

Intertek Testing Services Shenzhen Ltd. Guangzhou Branch

深圳天祥质量技术服务有限公司广州分公司

Room 02, 1-8/F & Room 01, E101/E201/E301/E401/E501/E601/E701/E801, 3/F Hengyun Building, 235 Kaifa Ave., Guangzhou
No.7-2, Caipin Road, Guangzhou Science City, GETDD, Guangzhou, China Economic & Technological Development District, Guangzhou, China
中国广州经济技术开发区科学城彩频路7号之二第1-8层02房、01房 中国广州经济技术开发区开发大道235号恒运大厦3楼
101、
E201、E301、E401、E501、E601、E701、E801
Tel: +86 20 8213 9001 Fax: +86 20 8208 9909 Postcode: 510663
Tel: +86 20 8396 6868 Fax: +86 20 8222 8169 Postcode: 510730





Test Report

Number: GZHT02286854

Summary of testing:

With reference to following standard:

- EN 14683:2019+AC:2019 Medical face masks – Requirements and test methods Type IIR

Materials Used in The Submitted Sample Were Found To Comply With The Type IIR Requirements of EN 14683:2019+AC:2019 with respect to Microbial Cleanliness, Bacterial Filtration Efficiency, Differential Pressure and Splash Resistance Pressure tests.

Prepared And Checked By:
For Intertek Testing Services Shenzhen Ltd. Guangzhou Branch

Lin Lin
General Manager



Ula / hilaryxu

Intertek Testing Services Shenzhen Ltd. Guangzhou Branch

深圳天祥质量技术服务有限公司广州分公司

Room 02, 1-8/F & Room 01, E101/E201/E301/E401/E501/E601/E701/E801, 3/F Hengyun Building, 235 Kaifa Ave., Guangzhou
 No.7-2, Caipin Road, Guangzhou Science City, GETDD, Guangzhou, China Economic & Technological Development District, Guangzhou, China
 中国广州经济技术开发区科学城彩频路7号之二第1-8层02房、01房 中国广州经济技术开发区开发大道235号恒运大厦3楼
 101、
 E201、E301、E401、E501、E601、E701、E801
 Tel: +86 20 8213 9001 Fax: +86 20 8208 9909 Postcode: 510663 Tel: +86 20 8396 6868 Fax: +86 20 8222 8169 Postcode: 510730



Test Report

Number: GZHT02286854

Tests Conducted (As Requested By The Applicant)

1 Microbial Cleanliness

As Per EN 14683:2019+AC:2019 Medical face masks-Requirements and test methods Annex D.

Test Item	Result (cfu/g)					Limit (cfu/g)
	(1)					
	Specimen 1	Specimen 2	Specimen 3	Specimen 4	Specimen 5	
Microbial cleanliness	<1#	<1#	<1#	<1#	<1#	Type IIR: ≤30

Remark:

cfu = Colony Forming Unit

≤ = Not More Than

= No Colony Was Detected At The Extraction Liquid Of The Samples.

Sample Received Condition: Sample In Closed Plastic Bag.

Tested Component:

(1) Blue Face Mask

- 2 Bacterial Filtration Efficiency (EN 14683:2019+AC:2019, Clause 5.2.2, Testing Refer To Annex B):
Flow rate: 28.3L/min, Test area: 77 cm², Test bacteria: Staphylococcus aureus ATCC 6538, Inside of the test mask was facing towards the challenge aerosol, The average plate count results of the positive controls: 2.6 x 10³ CFU, The average plate count results of the negative controls: <1 CFU.

Tested Sample	Result (%)	Performance Requirement for Medical Face Mask (%)
Specimen (1)	99.6	Type IIR : ≥ 98
Specimen (2)	99.5	
Specimen (3)	99.6	
Specimen (4)	99.7	
Specimen (5)	99.5	

Remark : Test was conducted by external provider.

Ula / hilaryxu





Test Report

Number: GZHT02286854

Tests Conducted (As Requested By The Applicant)

- 3 Differential Pressure (EN 14683:2019+AC:2019 Annex C):
Air flow: 8L/min, Test area diameter 25 mm, Test area: 4.9 cm².

<u>Tested Sample</u>	<u>Result (Pa/cm²)</u>	<u>Performance Requirement for Medical Face Mask (Pa/cm²)</u>
Specimen (1)	40.6	Type IIR: < 60
Specimen (2)	37.4	
Specimen (3)	48.6	
Specimen (4)	47.5	
Specimen (5)	41.5	
Average	43.1	

Remark : Test was conducted by external provider.

Ula / hilaryxu

Intertek Testing Services Shenzhen Ltd. Guangzhou Branch

深圳天祥质量技术服务有限公司广州分公司

Room 02, 1-8/F & Room 01, E101/E201/E301/E401/E501/E601/E701/E801, 6/F, Hengyun Building, 235 Kaifa Ave., Guangzhou
 No.7-2, Caipin Road, Guangzhou Science City, GETDD, Guangzhou, China Economic & Technological Development District, Guangzhou, China
 中国广州经济技术开发区科学城彩频路7号之二第1-8层02房、01房 中国广州经济技术开发区开发大道235号恒运大厦3楼
 101、
 E201、E301、E401、E501、E601、E701、E801
 Tel: +86 20 8213 9001 Fax: +86 20 8208 9909 Postcode: 510663 Tel: +86 20 8396 6868 Fax: +86 20 8222 8169 Postcode: 510730





Test Report

Number: GZHT02286854

Tests Conducted (As Requested By The Applicant)

4 Splash Resistance Pressure (ISO 22609:2004):

Synthetic Blood Surface Tension: 0.040 N/m, Distance Between Blow Head Front End And Target Area: 300 mm, Artificial Blood Volumes: 2 mL, Test Pressure: 16.0 kPa, Velocity: 550 cm/s, Use A Fixed Target.

<u>Tested Sample</u>	<u>Result</u>	<u>Performance Requirement for Medical Face Mask Type IIR:</u> No penetration at 16.0 kPa
Specimen (1)	None seen	
Specimen (2)	None seen	
Specimen (3)	None seen	
Specimen (4)	None seen	
Specimen (5)	None seen	
Specimen (6)	None seen	
Specimen (7)	None seen	
Specimen (8)	None seen	
Specimen (9)	None seen	
Specimen (10)	None seen	
Specimen (11)	None seen	
Specimen (12)	None seen	
Specimen (13)	None seen	

Remark : Test was conducted by external provider.

End of Report

This report is made solely on the basis of your instructions and/or information and materials supplied by you. It is not intended to be a recommendation for any particular course of action. Intertek does not accept a duty of care or any other responsibility to any person other than the Client in respect of this report and only accepts liability to the Client insofar as is expressly contained in the terms and conditions governing Intertek's provision of services to you. Intertek makes no warranties or representations either express or implied with respect to this report save as provided for in those terms and conditions. We have aimed to conduct the Review on a diligent and careful basis and we do not accept any liability to you for any loss arising out of or in connection with this report, in contract, tort, by statute or otherwise, except in the event of our gross negligence or wilful misconduct. No copy of the test report(except for full text copy) shall be made without the written approval by Intertek.

Ula / hilaryxu

Intertek Testing Services Shenzhen Ltd. Guangzhou Branch

深圳天祥质量技术服务有限公司广州分公司

Room 02, 1-8/F & Room 01, E101/E201/E301/E401/E501/E601/E701/E801, No.7-2, Caipin Road, Guangzhou Science City, GETDD, Guangzhou, China
 中国广州经济技术开发区科学城彩频路7号之二第1-8层02房、01房
 Hengyun Building, 235 Kaifa Ave., Guangzhou Economic & Technological Development District, Guangzhou, China
 中国广州经济技术开发区开发大道235号恒运大厦3楼

101、
 E201、E301、E401、E501、E601、E701、E801
 Tel: +86 20 8213 9001 Fax: +86 20 8208 9909 Postcode: 510663
 Tel: +86 20 8396 6868 Fax: +86 20 8222 8169 Postcode: 510730

